

Fig. 1

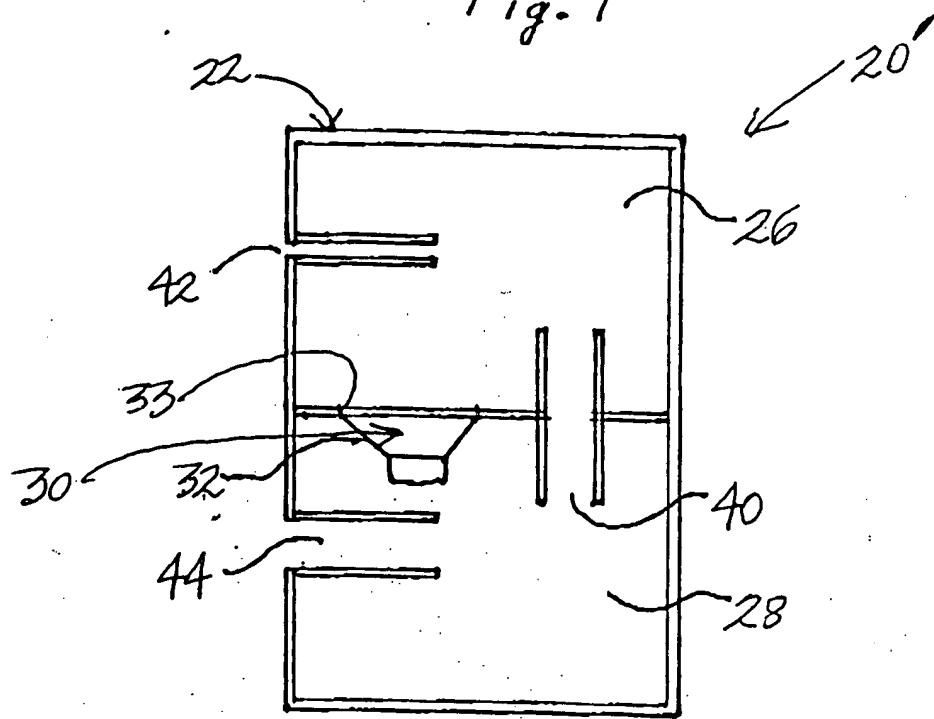


Fig. 4

File Editors Print View Options Windows Run AC Monte Carlo

AC

Gain

Db

0.00

GENSPK5E Temperature= 27 R1= 60.00001

Phase

Delay

Deg

Sec

360.0

10K

270.0 1K

180.0 100

90.0 10

0.0 1

-90.0 100m

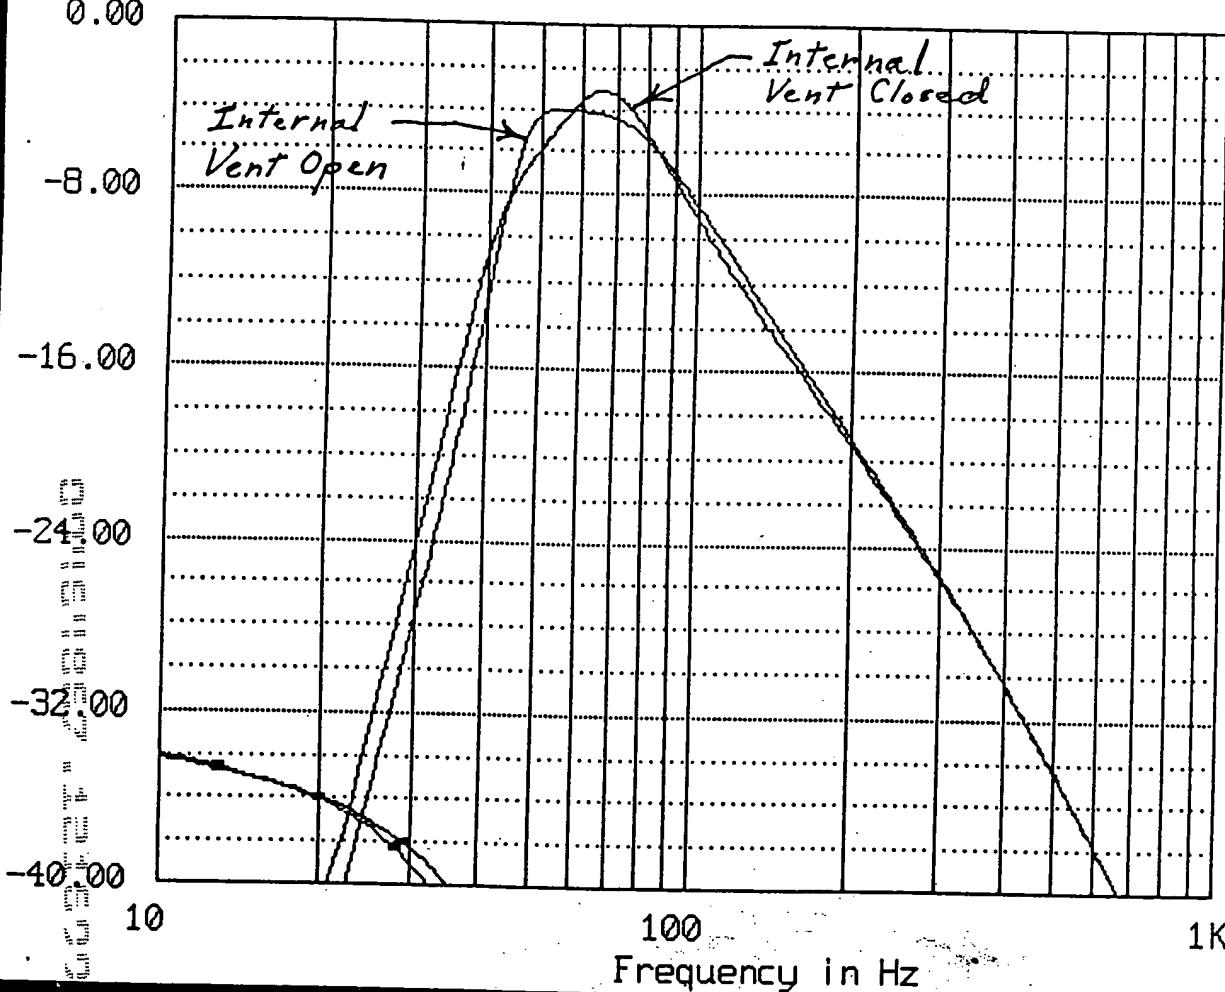


FIG. 2

File Editors Print View Options Windows Run AC Monte Carlo

Gain

Db

8.00

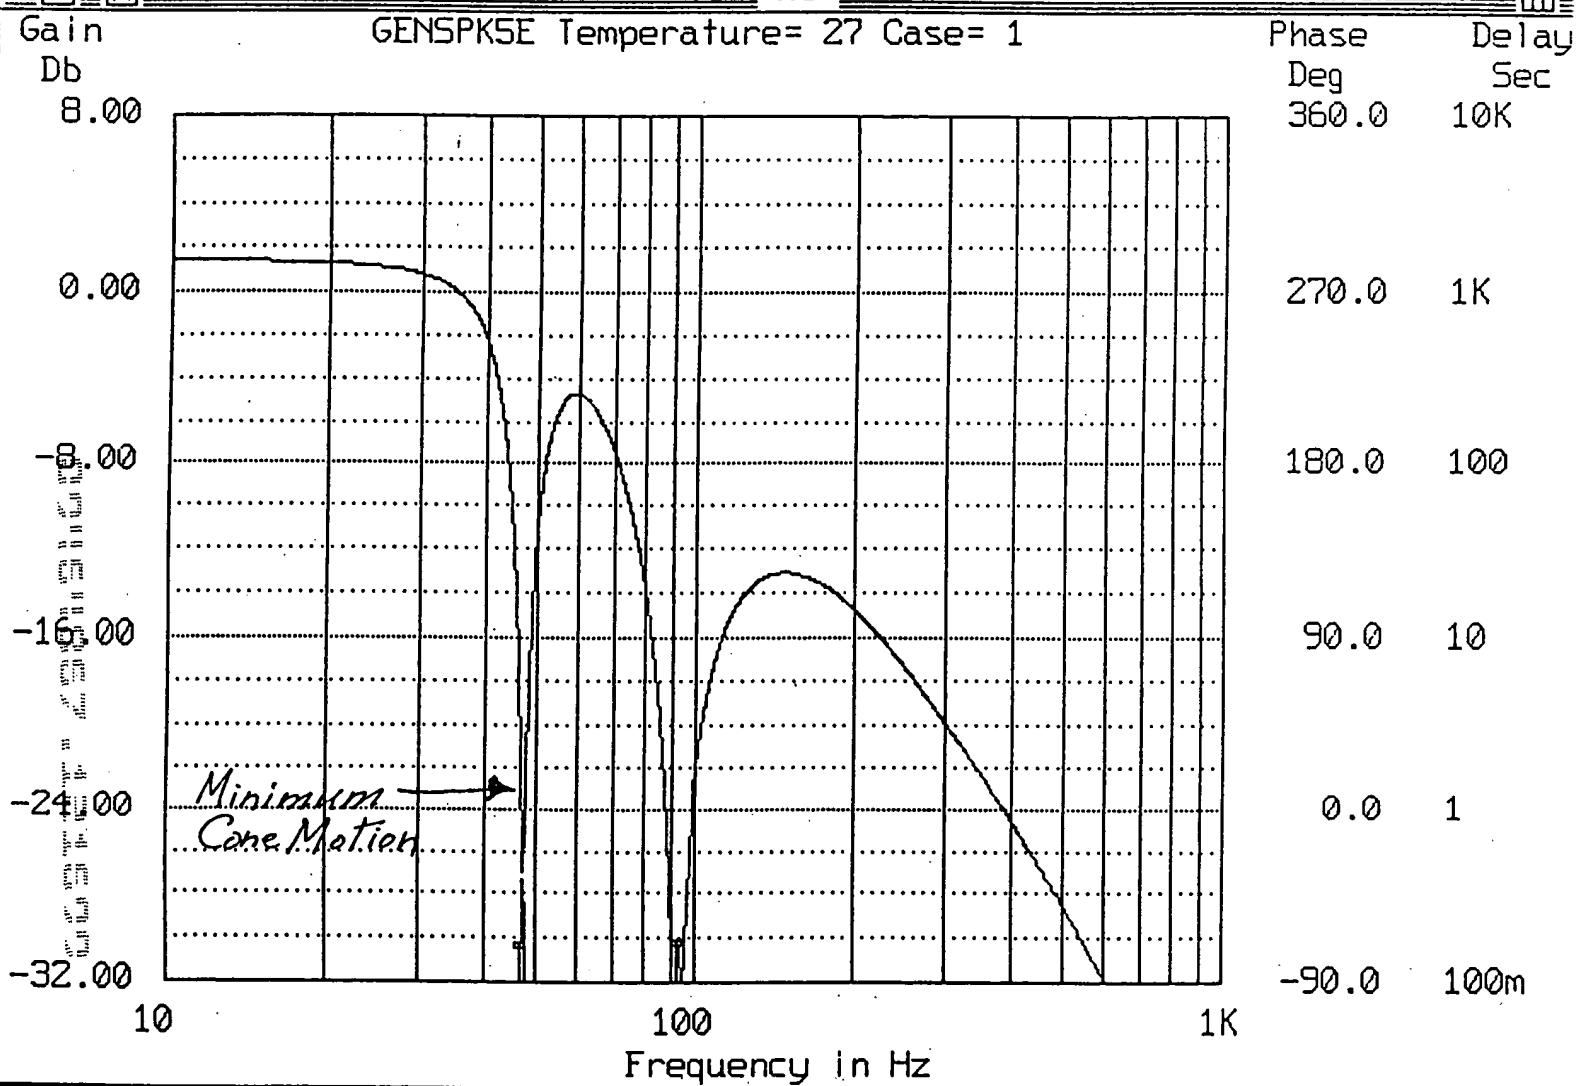


FIG. 3

File Editors Print View Options Windows Run AC Monte Carlo

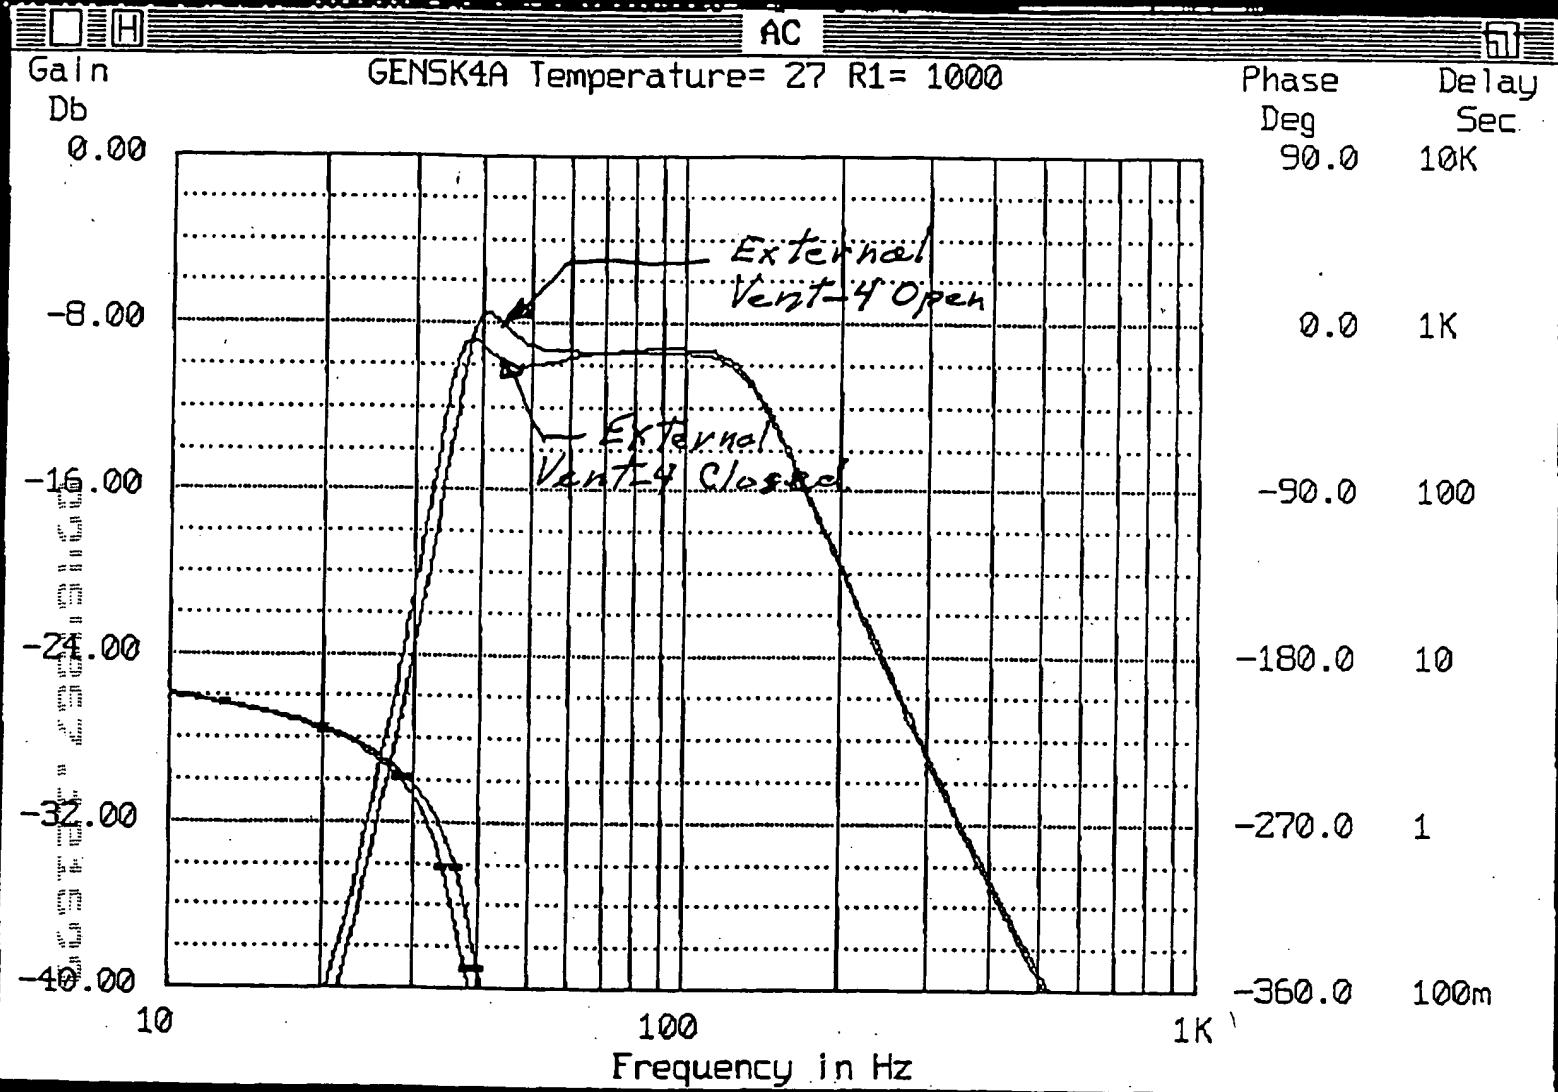


FIG. 5